


SALES DRAWING ONLY
NOT TO BE USED FOR MANUFACTURE

IMPORTANT

The sensor vent tube must be positioned so as to prevent direct ingress of moisture.
If located within a housing the housing must be vented to atmosphere

Alternatively

An extended vent tube (customer supply) must be fitted in areas where flooding or hose wash down are likely. 6mm (1/4") od plastic tube is suitable and should run to a dry area which is at the same atmospheric pressure as with in the tank.

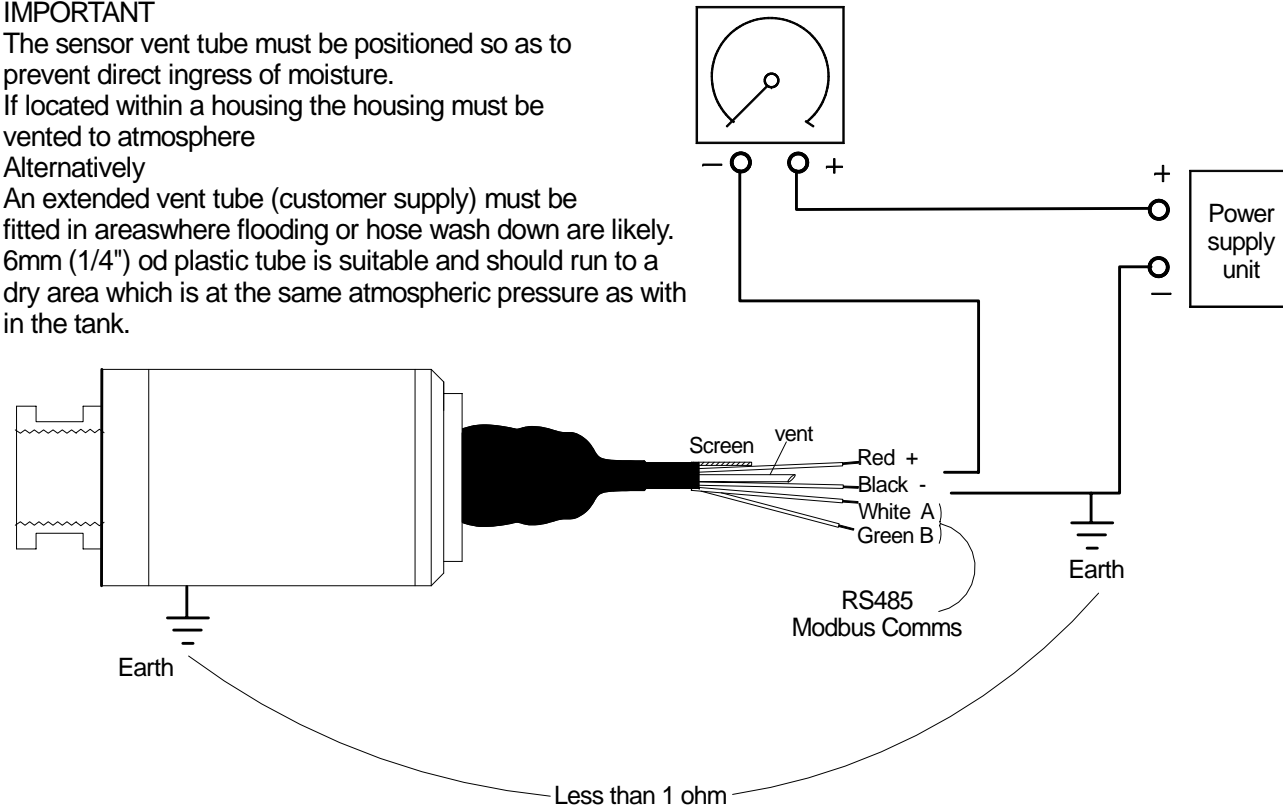

ISSUE	A
DATE	28-04-08
DCR	
DRAWN	JEK
CHECKED	

PSm Instrumentation Ltd

Haywards Heath, West Sussex RH16 1TW
ph: 44 (0) 1444 410040 f: 44 (0) 1444 410121
<http://www.psm-sensors.co.uk>

SCALE
NTS

UNLESS OTHERWISE STATED DIMENSIONS ARE IN
MILLIMETRES / INCHES

TITLE
**iCT Hookup
Drawing**

DRAWING NO
S-001309-iCT-GO

A4

SHT 1
OF 1